



OPEN ACCESS

ORIGINAL RESEARCH ARTICLE

Forced air warming during sedation in the cardiac catheterisation laboratory: a randomised controlled trial

Aaron Conway,^{1,2} Suzanna Ersotelos,³ Joanna Sutherland,^{4,5} Jed Duff⁶

¹Institute of Health and Biomedical Innovation, Queensland University of Technology, Brisbane, Queensland, Australia

²Cardiac Catheter Theatres, The Wesley Hospital, Brisbane, Queensland, Australia

³Cardiac Catheter Laboratory, St Vincent's Private Hospital, Sydney, Australia

⁴Department of Anaesthesia, Coffs Harbour Health Campus, Coffs Harbour, Australia

⁵Rural Clinical School, University of New South Wales, Coffs Harbour, New South Wales, Australia

⁶School of Nursing and Midwifery, University of Newcastle, Callaghan, New South Wales, Australia

Correspondence to

Dr Aaron Conway, The Wesley Hospital & Queensland University of Technology, Institute of Health and Biomedical Innovation, Kelvin Grove, QLD 4059, Australia; aaron.conway@qut.edu.au

Received 21 July 2017

Revised 19 September 2017

Accepted 21 September 2017

Published Online First

7 October 2017

ABSTRACT

Objective Forced air warming (FAW) during general anaesthesia is a safe and effective intervention used to reduce hypothermia. The objective of this study was to determine if FAW reduces hypothermia when used for procedures performed with sedation in the cardiac catheterisation laboratory.

Methods A parallel-group randomised controlled trial was conducted. Adults receiving sedation in a cardiac catheterisation laboratory at two sites were randomised to receive FAW or usual care, which involved passive warming with heated cotton blankets. Hypothermia, defined as a temperature less than 36°C measured with a sublingual digital thermometer after procedures, was the primary outcome. Other outcomes were postprocedure temperature, shivering, thermal comfort and major complications.

Results A total of 140 participants were randomised. Fewer participants who received FAW were hypothermic (39/70, 56% vs 48/69, 70%, difference 14%; adjusted RR 0.75, 95% CI=0.60 to 0.94), and body temperature was 0.3°C higher (95% CI=0.1 to 0.5, p=0.004). FAW increased thermal comfort (63/70, 90% vs 51/69, 74% difference 16%, RR 1.21, 95% CI=1.04 to 1.42). The incidence of shivering was similar (3/69, 4% vs 0/71 0%, difference 4%, 95% CI=-1.1 to 9.8). One patient in the control group required reintervention for bleeding. No other major complications occurred.

Conclusion FAW reduced hypothermia and improved thermal comfort. The difference in temperature between groups was modest and less than that observed in previous studies where use of FAW decreased risk of surgical complications. Therefore, it should not be considered clinically significant.

Trial registration number ACTRN12616000013460.

INTRODUCTION

Inadvertent perioperative hypothermia is considered an adverse effect of anaesthesia that should be avoided.¹ Forced air warming (FAW) is a safe and effective intervention for the prevention of inadvertent perioperative hypothermia.² It is recommended for use during general anaesthesia in clinical guidelines.²⁻³ The cardiac catheterisation laboratory (CCL) is similar to a perioperative environment in that patients are exposed for periods of time to low ambient room temperatures. Our recent review revealed that pharmacological agents used for procedural sedation and analgesia in the CCL, such as benzodiazepines, opioids and

propofol, impair normal thermoregulation, but not to the same extent as doses used for general anaesthesia.^{4,5} For example, studies in healthy volunteers have shown that propofol and opioids markedly reduced the vasoconstriction and shivering thresholds, producing a linear decrease in core temperature.⁶⁻⁸ Administration of midazolam only minimally impairs thermoregulatory control⁹ but did produce a dose-dependent decrease in temperature due to core to peripheral heat redistribution.¹⁰ We have previously identified a moderate prevalence of hypothermia (defined as body temperature <36.0°C) after procedures performed with sedation in a CCL where passive warming with heated (or non-heated) cotton blankets was used.¹¹

FAW increases body temperature during surgery in comparison with passive warming because it markedly reduces cutaneous heat loss. As a result, most patients who receive intraoperative FAW during surgery will meet the widely recommended goal for perioperative thermal management, which is for core temperature to be >36.0°C by the end of the procedure.¹² The extent to which application of FAW would increase temperature during procedures performed in the CCL with sedation is unknown. We aimed to determine whether FAW reduces hypothermia when used for procedures performed with sedation in the CCL.

METHODS

Design

A randomised controlled trial was conducted to compare FAW with passive warming using heated cotton blankets during elective procedures performed under sedation in a CCL. Full details of the protocol for this study have been published,¹³ and it was prospectively registered (ACTRN12616000013460). Informed consent was obtained from each participant, and the study protocol conforms to the 1975 Declaration of Helsinki as reflected by the university and hospital human research ethics committee approvals (UCH HREC 1505; QUT HREC 1500000643; SVH HREC 15/263).

Participants

Patients were eligible for inclusion if they were undergoing an interventional procedure of more than 30 min duration with sedation. Procedures were percutaneous coronary interventions, cardiovascular implantable electronic device procedures

Check for updates

To cite: Conway A, Ersotelos S, Sutherland J, et al. *Heart* 2018;**104**:685–690.

(eg, permanent pacemaker, implantable cardioverter-defibrillator), ablation of cardiac arrhythmias, structural heart procedures (patent foramen ovale and atrial septal defect closures, balloon aortic valvuloplasty) and peripheral angioplasty. The trial was conducted at two hospitals in Australia. Patients were ineligible if they were younger than 18 years, were not able to provide informed consent due to cognitive impairment or inability to understand and speak English or were febrile (temperature $>37.5^{\circ}\text{C}$).

Intervention and control groups

All participants received passive warming with heated cotton blankets, which were applied by the nurses as part of their usual practice. No restrictions on the use of passive warming were in place.

Intervention group participants received FAW during their procedures using a WarmTouch WT 6000 Warming Unit (Covidien, Minneapolis, Minnesota, USA) with either an 'upper body' or a 'lower body' blanket attachment. The temperature of the FAW unit was set at 45°C . Nursing staff monitored participants for signs of hyperthermia (sweating and flushed skin) and thermal discomfort so that the temperature of the device could be titrated according to a step-down protocol. An infrared aural canal thermometer was used to monitor temperature every 30 min so that active warming could be ceased if temperature rose above 37.5°C . Active warming was discontinued when procedures were completed.

Outcomes

The rate of hypothermia (temperature less than 36°C) at the conclusion of the procedure was the primary outcome. Other outcomes included postprocedure temperature, shivering, thermal comfort and major complications at 30 days postprocedure (defined as local infection that required reintervention or systemic infection/endocarditis, bleeding (symptomatic intracranial haemorrhage, clinically overt signs of bleeding associated with a drop in haemoglobin of more than 4 g/dL or fatal bleeding or required blood transfusion or procedural/surgical reintervention), cardiovascular complications (ventricular fibrillation, asystole, electromechanical dissociation or ventricular tachycardia without cardiac output that required cardiopulmonary resuscitation) and cardioversion or myocardial infarction (defined as confirmed myocardial infarction distinct from index event)).

Procedures

Allocation sequence generation

An independent statistician generated a stratified (by presence of an anaesthetist and site) block randomised sequence (two to four in each block). These strata were used to ensure that the use of propofol was balanced between groups.

Allocation concealment

The group allocations were concealed using sequentially ordered sealed opaque envelopes. The research assistant handed the envelope to the Scout nurse (nurse responsible for intraprocedural care) just prior to procedure commencement.

Data collection

Data collection was conducted blinded to group assignment. An oral digital thermometer placed in the sublingual pocket (Filac 3000 in direct measurement mode and calibrated according to the manufacturer's instructions) was used to measure temperature.

Temperatures were taken from the same site before and after procedures. Participants were observed after procedures to detect shivering, and researchers assessed thermal comfort on a 5-point scale (too cold, cool, just right, warm and too warm). Data about use of warming methods used in active and passive warming groups were collected. This included the number of times the temperature of the FAW device was titrated during procedures as well as the number of heated cotton blankets and towels used during and after procedures in the recovery area for both groups. Medical records were reviewed on discharge and readmission within the follow-up period.

Data analysis

Sample size

The sample size for this study was calculated to detect an 80% relative difference in the rate of hypothermia, which was the effect size observed in a previous study of this intervention during general anaesthesia.¹⁴ It was determined that 128 patients would be sufficient to detect an 80% relative reduction in hypothermia from 20% to 4% (type I error of 5% (two-tailed) and power of 80%). These estimates were drawn from our previous study.¹¹ A further 10% was recruited in case of cross-over and dropout, making the total sample size of 140 participants.

Statistical analysis

Intention-to-treat principles were used in the analyses. Absolute differences as well as relative risks with 95% CIs were calculated for the primary outcome of hypothermia and the secondary outcome of thermal comfort (classified as a rating of 'just right') using Poisson regression with robust variance estimation to adjust for the stratified variables (site and use of monitored anaesthesia care) as well as preprocedural temperature.¹⁵ As there were too few events to use a regression model to compare the rates of shivering between groups, a Fisher's exact test was used without adjustment for stratification. Analysis of covariance, adjusting for baseline temperature and stratification variables, was used to compare postprocedure temperatures. A subgroup analysis was conducted by including an interaction term in the model for use of propofol.

RESULTS

There were 598 patients screened for eligibility between April 2016 and March 2017 (figure 1). The major reasons patients were not enrolled in the study included the use of general anaesthesia (n=88) or an anticipated procedural duration of less than 30 min (n=341). A total of 140 participants were randomised. Demographic and clinical characteristics are presented in table 1.

Warming methods

The temperature of the FAW device was titrated down during the procedure in accordance with the step-down protocol for eight of the intervention group participants. One patient randomised to the control group undergoing an electrophysiology procedure received FAW at the discretion of the anaesthetist because the patient expressed thermal discomfort prior to procedure commencement. Nurses used a total of 150 heated cotton blankets and 36 heated towels during and after procedures for the 69 participants randomised to the control group. Nurses used 115 heated blankets and 37 heated towels during and after procedures for the 71 participants randomised to the intervention group.

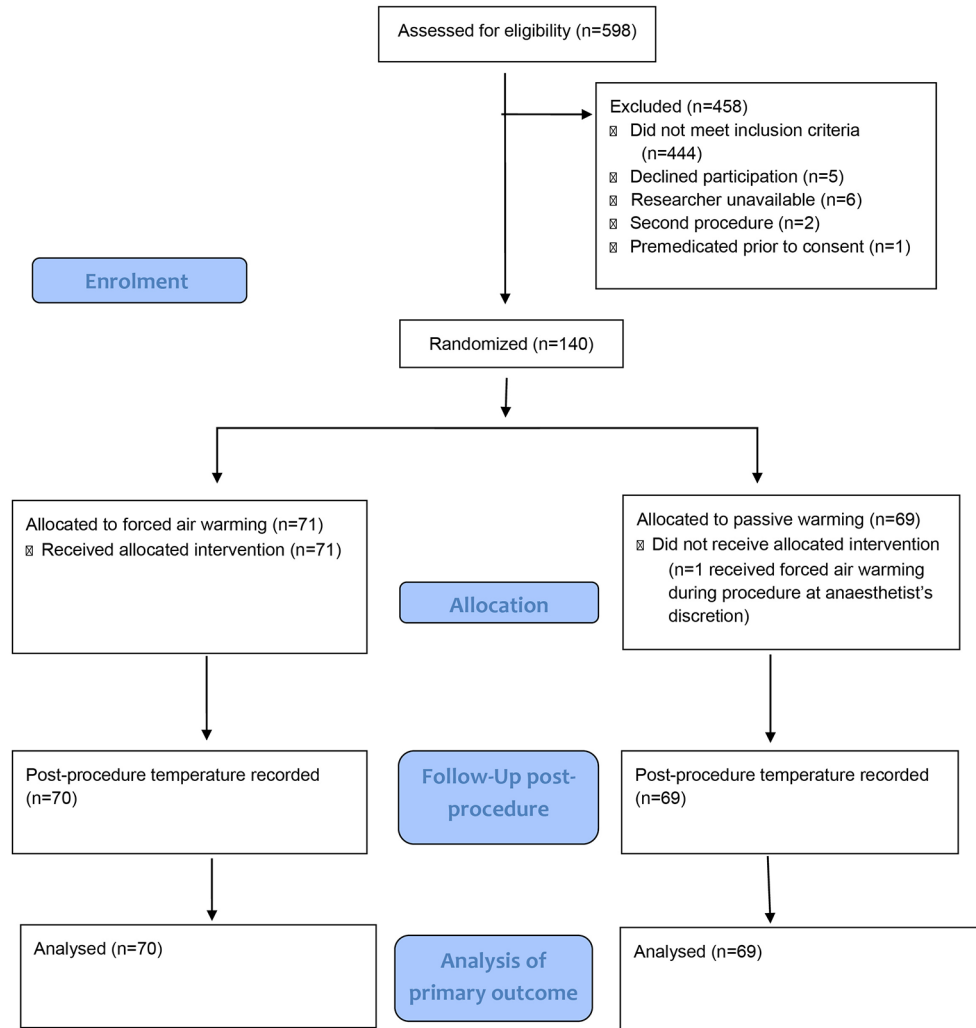


Figure 1 Trial diagram.

Primary outcome

Fewer participants who received FAW were hypothermic (39/70, 56% vs 48/69, 70%, difference 14%) after their procedures. This difference was statistically significant in the model with adjustment for variables used for stratification and baseline temperature (adjusted RR 0.75, 95% CI=0.60 to 0.94, $p=0.011$).

Secondary outcomes

Body temperature was 0.3°C higher (95% CI=-0.5 to -0.1, $p=0.004$) in the FAW group (table 2). The interaction between allocation group and use of propofol was not significant ($p=0.564$).

Forced air warming reduced shivering (0/71 0% vs 3/69, 4%, difference 4%, 95% CI=-1.1 to 9.8, $p=0.117$) and increased self-reported thermal comfort (63/70, 90% vs 51/69, 74% difference 16%, adjusted RR 1.21, 95% CI=1.04 to 1.42, $p=0.014$). One patient in the control group required reintervention for bleeding. No major infections or cardiovascular complications occurred in either group. There was no evidence of thermal injury to skin after procedures in the FAW group.

DISCUSSION

Using FAW during interventional procedures performed with sedation in the CCL decreased rates of hypothermia by 14% (a 25% relative risk reduction) as a result of increasing temperature

by 0.3°C on average compared with passive warming. The increase in body temperature in the FAW group should be considered modest. It is similar to those arising from testing of this intervention with sedated patients in controlled experimental conditions¹⁶ and with application of active warming during neuraxial anaesthesia.¹⁷ A recent meta-analysis of eight trials with 1189 participants who received neuraxial anaesthesia found that active warming increased postoperative temperature by 0.36°C in comparison with passive warming (95% CI=0.16 to 0.55) and reduced risk of hypothermia by 29% (RR 0.71, 95% CI=0.61 to 0.83).¹⁷

A positive effect of active warming in our trial was increased thermal comfort. This result is consistent with a meta-analysis conducted in a recent Cochrane review.¹⁸ Active body surface warming increased ratings of thermal comfort in a meta-analysis of four trials with 364 participants (standardised mean difference 0.72, 95% CI=0.29 to 1.24).¹⁸ The relative contributions to thermal comfort of core and skin temperatures is about equal.¹⁹ As such, our finding that FAW increased ratings of thermal comfort in comparison with passive warming would be due to the effect of this device on skin temperature in addition to the 0.3°C increase in body temperature that was induced.

The increase in temperature in the group of participants randomised to receive FAW in our trial was less than that observed

Table 1 Baseline characteristics

Variable	Forced air warming (n=71), mean (SD) or n (%)	Passive warming (n=69), mean (SD) or n (%)
Age	72 (13)	73 (13)
Males	49 (69)	44 (64)
BMI	27 (5)	27 (6)
Charlson Comorbidity Score	1.6 (1.6)	1.8 (2.2)
ASA class >2	64 (90)	62 (90)
Procedure duration (min)	57 (39)	56 (29)
PCI	16 (23)	16 (23)
Cardiac implantable electronic device	34 (48)	32 (46)
Electrophysiology study and/or ablation of cardiac arrhythmia	8 (11)	7 (10)
Peripheral intervention	8 (11)	9 (13)
Structural heart procedure	5 (7)	5 (7)
Monitored anaesthesia care	34 (48)	33 (48)
Propofol used	27 (38)	29 (42)
Total midazolam dose	2.1 (0.9)	2 (0.9)
Total fentanyl dose	50 (35)	45 (32)
Propofol bolus amount	43 (88)	38 (81)
Propofol target controlled infusion used	9 (13)	9 (13)
Room temperature	19.8 (1.0)	20 (1.1)

ASA, American Society of Anesthesiologists; BMI, body mass index; PCI, percutaneous coronary intervention.

in previous studies where the use of this intervention decreased risk of surgical complications.^{20 21} It is likely that the underlying mechanisms for the protective effects of active warming on surgical outcomes are influenced by the degree to which core temperature is increased. For example, the relationship between core temperature and immune function is implicated in the development of postoperative infection.²² Moreover, recent research has shown that greater reductions in temperature during surgery were associated with increased likelihood of blood transfusion requirement.¹² It is therefore not likely that increasing temperature with FAW by only a few tenths of a degree during sedation would improve clinical outcomes for this population.

It should be noted that the average preoperative temperature was low in our sample, at about 36.1°C. A recent analysis of preoperative temperatures from seven prospective studies

also revealed an unexpectedly high incidence of preoperative hypothermia.²³ In this analysis, independent predictors of preoperative hypothermia were male sex and being aged over 52 years.²³ The majority of participants included in our sample were male (66%), and the average age was 72. As such, the demographic characteristics of our sample likely explain the low preoperative temperatures that were observed. As the average preprocedural temperature was low, further research on the added benefit of preoperative warming on patients undergoing sedation in the CCL may be warranted. In a recent Cochrane Review on the effectiveness of active warming for preventing hypothermia in surgical patients, the authors concluded that the addition of preoperative full-body warming for a period of 30 min had an extra protective benefit over intraoperative warming.¹⁸ Several other studies highlight the role of preoperative warming for preventing perioperative hypothermia.^{24 25}

Limitations

The rates of hypothermia used for the sample size calculation were different to those observed in our study. We attribute this to the type of thermometer used. There was a lower incidence of postprocedural hypothermia observed in our previous study where an infrared aural canal thermometer was used.¹¹ We used a sublingual digital thermometer in this randomised controlled trial because it is a more accurate non-invasive temperature measuring device for postanaesthetic patients compared with infrared aural canal thermometers.²⁶

A further potential limitation is that we did not blind participants or clinicians to group assignment. The technical challenges of achieving double blinding in trials of warming strategies have been acknowledged previously.²⁷ Importantly, outcome assessors were blinded to group assignment to reduce the risk of detection bias in our trial.

It should also be noted that we only included patients undergoing procedures with an anticipated duration of more than 30 min. Extrapolation of our findings to other procedures performed in procedural settings is not recommended, as it is likely that the effect of FAW on body temperature is dependent on contextual factors, including the length of procedures and ambient temperature to which the patients have been exposed. The ambient temperature during procedures was 20°C on average. Active warming may have less of an effect on body temperature and thermal comfort in comparison with passive

Table 2 Effect of forced air warming on temperature (°C) for the main comparison and use of propofol subgroup analysis

		Forced air warming	Passive warming	Difference between means (95% CI)	p Value	p Value for interaction
Total	Baseline	36.1 (0.5)	36.2 (0.5)	0.1		
	Postprocedure	35.8 (0.7)	35.6 (0.7)	-0.2 (-0.4 to 0.01)	0.07	
	ANCOVA (adjusting for baseline temperature and stratification variables)			-0.3 (-0.5 to -0.1)	0.004	
Propofol used	Baseline	36 (0.3)	36.1 (0.4)	0.1		
	Postprocedure	35.6 (0.4)	35.5 (0.5)	-0.1 (-0.4 to 0.1)	0.185	
	ANCOVA (adjusting for baseline temperature and stratification variables)			-0.2 (-0.4 to -0.02)	0.033	
Propofol not used	Baseline	36.1 (0.5)	36.2 (0.5)	0.1		0.564
	Postprocedure	35.9	35.7	-0.2 (-0.6 to -0.1)	0.194	
	ANCOVA (adjusting for baseline temperature and stratification variables)			-0.3 (-0.6 to -0.01)	0.04	

ANCOVA, analysis of covariance.

Key messages

What is already known on this subject?

The pharmacological agents used for procedural sedation and analgesia in the cardiac catheterisation laboratory impair normal thermoregulation. As a result, inadvertent hypothermia (defined as body temperature $<36.0^{\circ}\text{C}$) is common after procedures performed with sedation in a cardiac catheterisation laboratory.

What might this study add?

Using forced air warming during interventional procedures performed with sedation in the cardiac catheterisation laboratory decreased rates of hypothermia by 14% as a result of increasing temperature by 0.3°C on average compared with passive warming. Forced air warming also increased thermal comfort.

How might this impact on clinical practice?

Using forced air warming during procedures performed with sedation in the cardiac catheterisation laboratory would reduce postprocedural hypothermia (temperature $<36.0^{\circ}\text{C}$) and improve thermal comfort. However, it is unlikely that increasing temperature by only a few tenths of a degree with active warming will improve clinical outcomes.

warming in procedural suites where the ambient temperature is higher.

One patient in the control group received FAW, and postprocedural temperature could not be measured using the sublingual thermometer for one participant. This small dropout and cross-over rate is unlikely to have exerted a major impact on our estimates of the effect of FAW on temperature and thermal comfort during sedation in the CCL. Based on the data collected about the amount of passive warming used in both intervention and control groups, we do not suspect there was any significant bias associated with suboptimal application of passive warming in the control group.

CONCLUSIONS

FAW can be recommended for use during procedures performed with sedation in the CCL to reduce postprocedural hypothermia and to improve thermal comfort. However, the difference in temperature between active and passively warmed patients is not clinically important, as it is unlikely that increasing temperature by only a few tenths of a degree will reduce risk of procedural complications.

Contributors AC, JD and JS designed the study. AC and SE collected data. AC analysed the data and wrote the first draft of the manuscript. All authors contributed important intellectual content to the drafted manuscript and approved it for publication.

Funding Dr AC was awarded an NHMRC Early Career Fellowship to conduct this study and other related research (APP1091657). This study is funded by a St Vincent's Clinic Foundation Multidisciplinary Patient Focussed Research Grant. Equipment for the study has been awarded by the Covidien Investigator Sponsored Research Program.

Competing interests None declared.

Patient consent Obtained.

Ethics approval Informed consent was obtained from each participant, and the study protocol conforms to the 1975 Declaration of Helsinki as reflected by the university and hospital human research ethics committee approvals (UCH HREC 1505; QUT HREC 1500000643; SVH HREC 15/263).

Provenance and peer review Not commissioned; externally peer reviewed.

Open Access This is an Open Access article distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 4.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited and the use is non-commercial. See: <http://creativecommons.org/licenses/by-nc/4.0/>

© Article author(s) (or their employer(s) unless otherwise stated in the text of the article) 2018. All rights reserved. No commercial use is permitted unless otherwise expressly granted.

REFERENCES

- Sessler DI. Perioperative thermoregulation and heat balance. *Lancet* 2016;387:2655–64.
- NICE. *The management of inadvertent perioperative hypothermia in adults*. UK: National Institute for Health and Care Excellence, 2008.
- Torossian A, Bräuer A, Höcker J, et al. Preventing inadvertent perioperative hypothermia. *Dtsch Arztebl Int* 2015;112:166.
- Conway A, Rolley JX, Page K, et al. Trends in nurse-administered procedural sedation and analgesia across Australian and New Zealand cardiac catheterisation laboratories: results of an electronic survey. *Aust Crit Care* 2014;27:4–10.
- Conway A. A review of the effects of sedation on thermoregulation: insights for the cardiac catheterisation laboratory. *J Perianesth Nurs* 2016;31:226–36.
- Matsukawa T, Kurz A, Sessler DI, et al. Propofol linearly reduces the vasoconstriction and shivering thresholds. *Anesthesiology* 1995;82:1169–80.
- Leslie K, Sessler DI, Bjorksten AR, et al. Propofol causes a dose-dependent decrease in the thermoregulatory threshold for vasoconstriction but has little effect on sweating. *Anesthesiology* 1994;81:353–60.
- Kurz A, Go JC, Sessler DI, et al. Alfentanil slightly increases the sweating threshold and markedly reduces the vasoconstriction and shivering thresholds. *Anesthesiology* 1995;83:293–9.
- Kurz A, Sessler DI, Annadara R, et al. Midazolam minimally impairs thermoregulatory control. *Anesth Analg* 1995;81:393–8.
- Matsukawa T, Hanagata K, Ozaki M, et al. I.m. midazolam as premedication produces a concentration-dependent decrease in core temperature in male volunteers. *Br J Anaesth* 1997;78:396–9.
- Conway A, Kennedy W, Sutherland J. Inadvertent hypothermia after procedural sedation and analgesia in a cardiac catheterisation laboratory: a prospective observational study. *J Cardiothorac Vasc Anesth* 2015;29:1285–90.
- Sun Z, Honar H, Sessler DI, et al. Intraoperative core temperature patterns, transfusion requirement, and hospital duration in patients warmed with forced air. *Anesthesiology* 2015;122:276–85.
- Conway A, Duff J. Forced air warming to maintain normothermia during sedation in the cardiac catheterization laboratory: protocol for the THERMISED pilot randomized controlled trial. *J Adv Nurs* 2016;72:2547–57.
- Horn EP, Bein B, Böhm R, et al. The effect of short time periods of pre-operative warming in the prevention of peri-operative hypothermia. *Anaesthesia* 2012;67:612–7.
- Zou G. A modified poisson regression approach to prospective studies with binary data. *Am J Epidemiol* 2004;159:702–6.
- Sato H, Yamakage M, Okuyama K, et al. Forced-air warming effectively prevents midazolam-induced core hypothermia in volunteers. *Eur J Anaesthesiol* 2009;26:566–71.
- Shaw CA, Steelman VM, DeBerg J, et al. Effectiveness of active and passive warming for the prevention of inadvertent hypothermia in patients receiving neuraxial anesthesia: a systematic review and meta-analysis of randomized controlled trials. *J Clin Anesth* 2017;38:93–104.
- Madrid E, Urrutia G, Roqué i Figuls M, et al. Active body surface warming systems for preventing complications caused by inadvertent perioperative hypothermia in adults. *Cochrane Database Syst Rev* 2016;4:CD009016.
- Frank SM, Raja SN, Bulcao CF, et al. Relative contribution of core and cutaneous temperatures to thermal comfort and autonomic responses in humans. *J Appl Physiol* 1999;86:1588–93.
- Kurz A, Sessler DI, Lenhardt R. Perioperative normothermia to reduce the incidence of surgical-wound infection and shorten hospitalization. *N Engl J Med* 1996;334:1209–16.
- Schmied H, Kurz A, Sessler DI, et al. Mild hypothermia increases blood loss and transfusion requirements during total hip arthroplasty. *Lancet* 1996;347:289–92.
- Wenisch C, Narz E, Sessler DI, et al. Mild intraoperative hypothermia reduces production of reactive oxygen intermediates by polymorphonuclear leukocytes. *Anesth Analg* 1996;82:810–6.
- Wetz AJ, Perl T, Brandes IF, et al. Unexpectedly high incidence of hypothermia before induction of anesthesia in elective surgical patients. *J Clin Anesth* 2016;34:282–9.
- Horn EP, Bein B, Broch O, et al. Warming before and after epidural block before general anaesthesia for major abdominal surgery prevents perioperative hypothermia: a randomised controlled trial. *Eur J Anaesthesiol* 2016;33:334–40.

- 25 Steelman VM, Perkhounkova YS, Lemke JH. The gap between compliance with the quality performance measure "perioperative temperature management" and normothermia. *Journal for healthcare quality : official publication of the national. J Healthcare Qual* 2015;37:333–41.
- 26 Langham GE, Maheshwari A, Contrera K, *et al.* Noninvasive temperature monitoring in postanesthesia care units. *Anesthesiology* 2009;111:90–6.
- 27 Akhtar Z, Hesler BD, Fiffick AN, *et al.* A randomized trial of prewarming on patient satisfaction and thermal comfort in outpatient surgery. *J Clin Anesth* 2016;33:376–85.